

Balloon Specification

Part NO.	Initial Length (mm)	PSI Rating	Max. Inflation Volume(cc)	Maximum Diameter(mm)	Maximum Length(mm)
Spino Balloon 15	15	300	4	17	22

POP kit Composition

NO.	Description	POP-A	POP-B
1	Opturator	1ea	1ea
2	Cannula	2ea	1ea
3	Bone Drill	1ea	1ea
4	Cement Injection Device	6ea	3ea
5	Guide Wire	2ea	1ea

Kyphoplasty Balloon Catheter System

Spino Balloon™



Indication


- VCF(Vertebral Compression fracture) due to Osteoporosis
- Osteolytic fracture
- Metastatic bone fractures

Manufactured by **SG SURGI BIO**

SURGIBIO Co., Ltd. 407#, SUNTECHCITY, 474, DUNCHON-DAERO,
JUNGWON-GU, SEONGNAM-SI, GYEONGGI-DO, KOREA.

Tel : 82-31-747-1527 E-mail : surgitech@naver.com

Spino Balloon™ Balloon Catheter 15

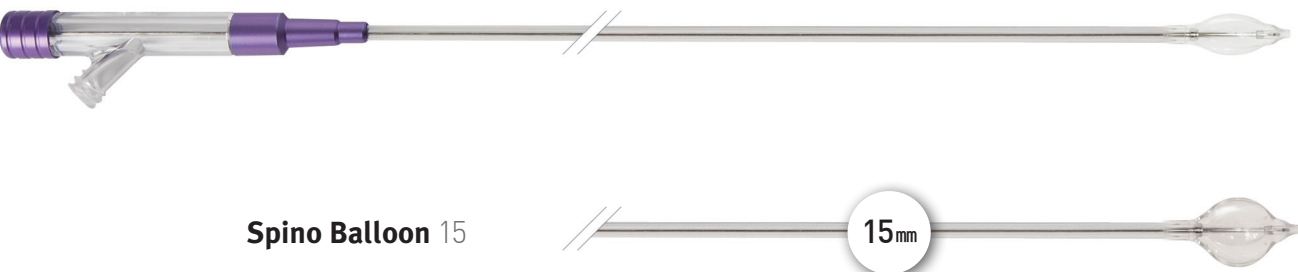


Spino Balloon 15

Special Feature

- Easy to inflate and Variety size

Radiflator™ Balloon Inflation Device

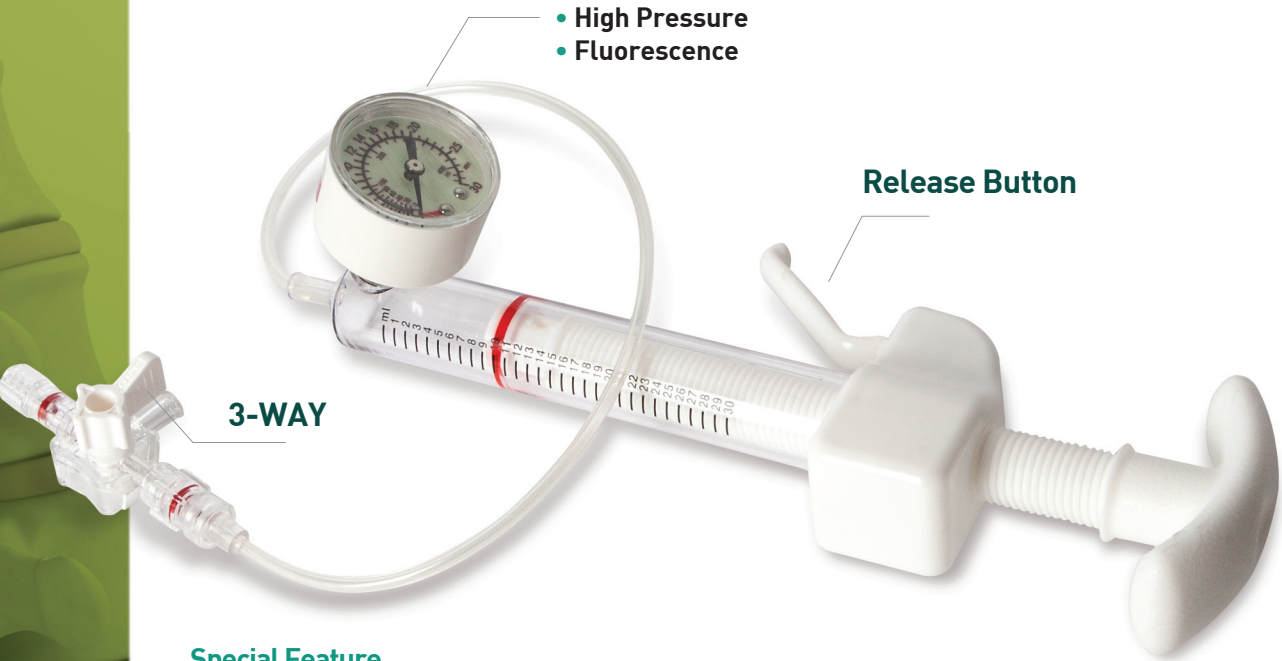

- High Pressure
- Fluorescence

Release Button


3-WAY

Special Feature


- Easy to inflate and Fluorescence

POP-A™ (Percutaneous Osteo Plasty) System

1. Opturator / Cannula

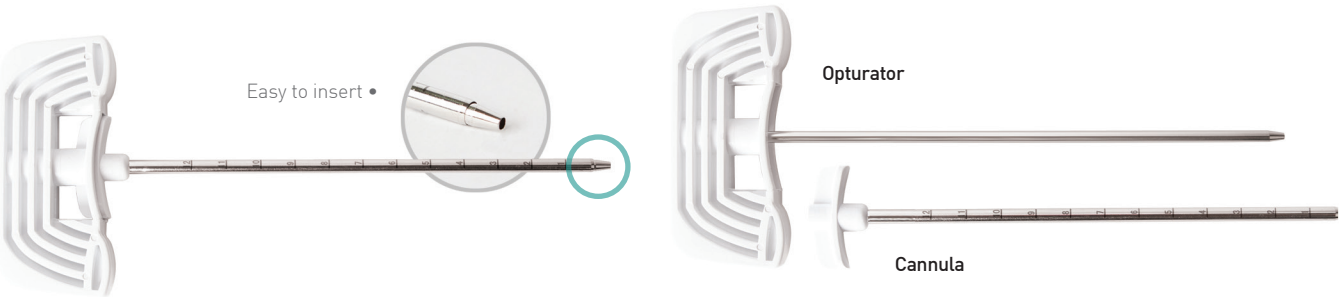

2. Bone Drill

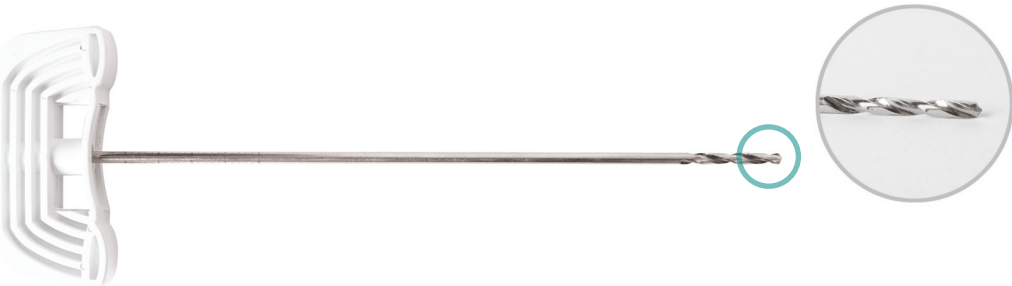

3. Cement Injection Device



4. Guide wire



Bonjector™ Bone Marrow Needle Bonjector 11 / Bonjector 13

